


Beacon 800
Detector/Transmitter
Terminal Strip

BEACON 800 HOUSING

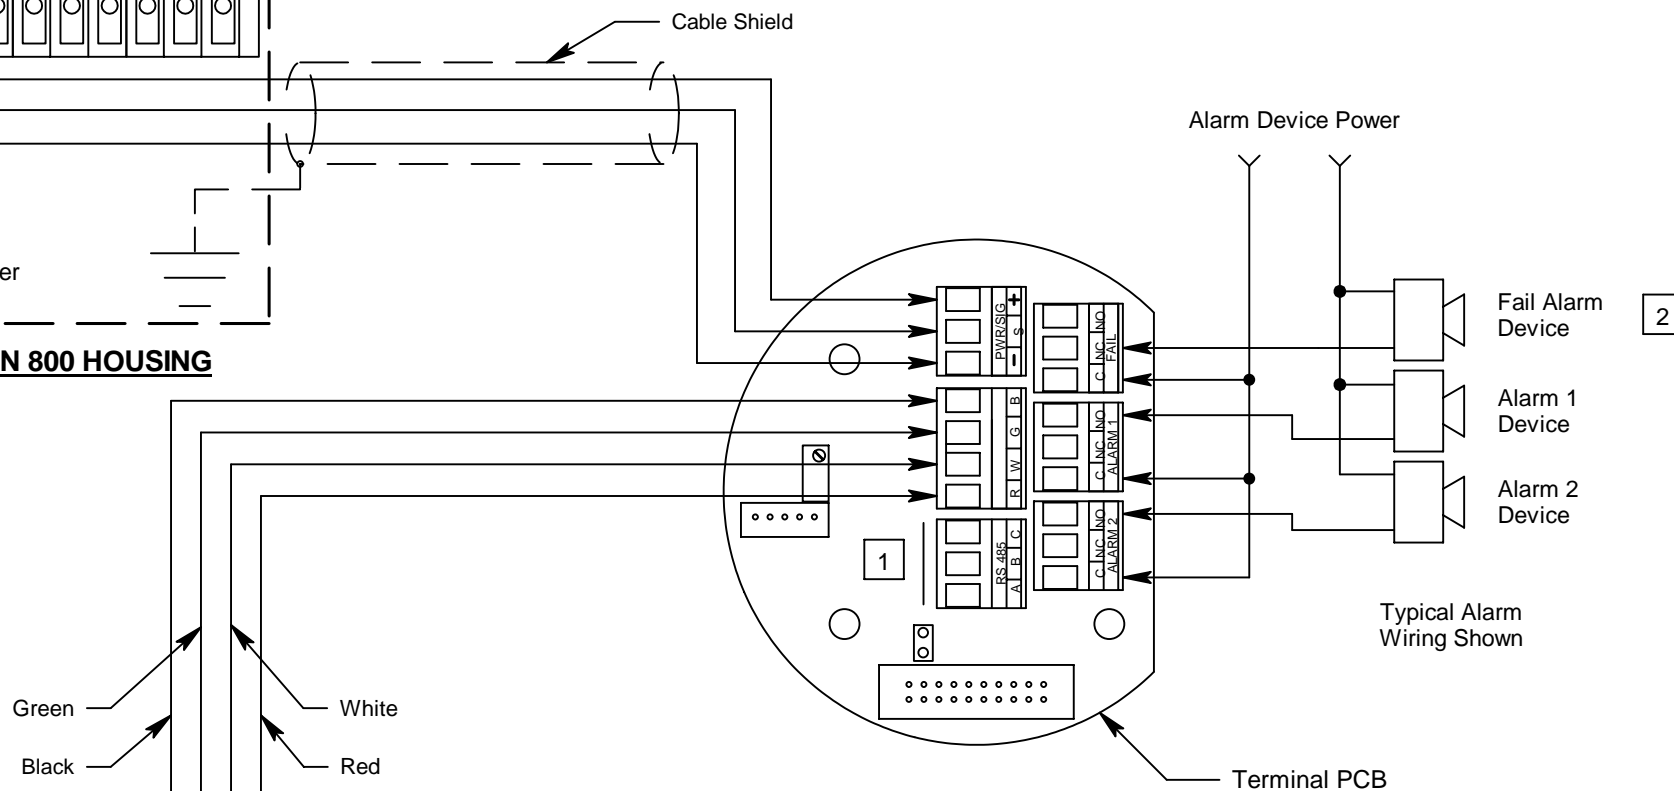

Notes

- [1] See drawing 65-2610RK-R10 for RS-485 wiring.
[2] Each set of relay contacts rated for 5 amps 250 VAC resistive.

IR CO2 Detector

DO NOT SCALE DRAWING	
Deburr	Break Edges .010 R
Tolerances & Finishes Unless Otherwise Noted:	
.XX ± .010	Angles ± 0° 30'
.XXX ± .005	Conc. .010 TIR
Fractions ± .015	Finish 125/32
Finish for O-ring Grooves, 3 Sides	

All Dimensions In Inches Unless Otherwise Noted.

MATERIAL: N/A

FINISH: N/A

SCALE: None



RKI Instruments, Inc.
www.rkiinstruments.com

TITLE: Wiring Diagram , M2, IR CO2 to Beacon 800

A

DRAWN
BY: KMP

PART NUMBER:
65-2630RK-03-R04

REVISION:
P1

APPROVED BY:

DATE: 3/22/06

PAGE 1 OF 1